


# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska


Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program


Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130187
Name	DAN PASQUARIELLO	ID#	2620 Date 3-24-12
A	Agency	DILLINGHAM PD	Phone # 842-5354
	Instrument Location	DILLINGHAM PD	
B	Alco S/N	58428	Target Value .080 High Pressure 900 PSI
	Alco Test Values	.077 1st Alco	.078 2nd Alco
	Signature		
(OVER)			


(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

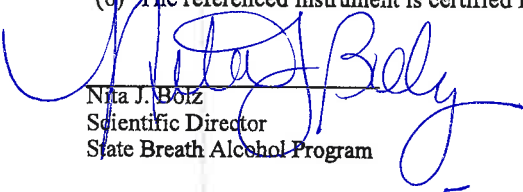  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 5 day of April, 2012. 

  
Daniel L. Nicholas (Notary Seal Stamp)  
Notary Public, State of Alaska  
Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130187

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130187

MARCH 24, 2012

OPERATOR'S NAME:  
PASQUARIELLO, DAN  
OPERATOR'S NUMBER: 2620  
SUBJECT'S LAST NAME:  
VORC  
SUBJECT'S FIRST NAME/MI :  
VORC

O.L. #: 1234567890  
DEPT/AGENCY: DLG1  
CASE/REPORT: 1234567890  
TEST TYPE: U  
ALCO TARGET VALUE: .000  
ALCO S/N: 50428

### — BREATH ANALYSIS —

.000 ADJUSTED FOR 30.11 in  
ALCO TARGET .000 13:40  
BLANK TEST .000 13:41  
INTERNAL STANDARD VERIFIED 13:41  
ALCO TO 30.11 in .077 13:41  
BLANK TEST .000 13:42  
SUBJECT SAMPLE .000 13:43  
BLANK TEST .000 13:43  
ALCO TO 30.11 in .078 13:44  
BLANK TEST .000 13:45

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130187

MARCH 24, 2012  
TIME 13:45

### — DIAGNOSTIC CHECK —

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 41c  
BAROMETER: 30.11 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

!@#%&'()\*+,-./0123456789:;<=>?AB CDEFG  
HIJKLMNOPQRSTUVWXYZ[\]^\_`abcdefgijklmno  
pqrstuvwxyz{|}~